


# CLEANSTREAM H3000

Liquid-to-Liquid In-Line Heater for High Temperature Baths

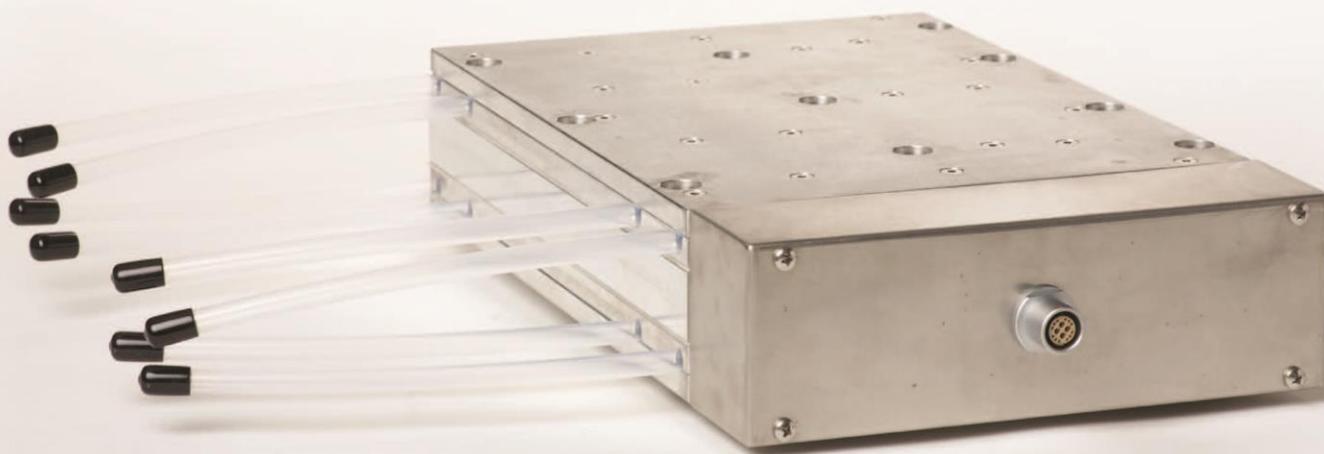

**Product Manual**

**EC Declaration of Conformity**

We Solid State Cooling Systems  
 167 Myers Corners Road  
 Wappingers Falls, NY 12592  
 USA

declare under sole responsibility that the

Cleanstream H3000 (with Hummel electrical connectors)

complies with the essential requirements, Annex 1, of Low Voltage Directive 2006/95/EC.  
 Compliance was demonstrated to the following specifications as listed in the official Journal of the  
 European Communities:

EN 61010-1 +A1+A2: 1995	Low Voltage Directive safety requirements for electrical equipment for measurement, control, and laboratory use.
IEC 61010-1:2010 (Third Edition) / EN 61010-1:2010	Safety requirements for electrical equipment for measurement, control, and laboratory use

Equipment Description: Process heating and cooling equipment with no moving parts.

Lloyd F Wright CTO	
Date	August 12, 2016

## TABLE OF CONTENTS

<b>Symbols Used in this Manual .....</b>	<b>2</b>
<b>1.0 Introduction .....</b>	<b>3</b>
<b>2.0 Specifications .....</b>	<b>4</b>
<b>3.0 Installation .....</b>	<b>6</b>
<b>3.1 Electrical Connections .....</b>	<b>6</b>
<b>3.2 - Plumbing Connections .....</b>	<b>8</b>
<b>3.3 - Mechanical Layout/Mounting .....</b>	<b>8</b>
<b>3.4 – Recommended Safety Precautions.....</b>	<b>9</b>
<b>4.0 Start-Up/Operation .....</b>	<b>12</b>
<b>5.0 Maintenance .....</b>	<b>13</b>
<b>6.0 Lockout/Tag-out .....</b>	<b>13</b>
<b>7.0 Technical Support .....</b>	<b>14</b>
<b>Warranty Policy .....</b>	<b>15</b>

## SYMBOLS USED IN THIS MANUAL



To avoid electric shock, disconnect all power prior to servicing. The power supply DC output is not isolated from the AC input. Input power must be disconnected to prevent hazardous potentials (approximately 145 volts) from appearing on the output, even when voltage between output terminals is zero.



*Burn Hazard -- Hot Surface.* Top and bottom surface temperatures of the Cleanstream H3000 may reach 150 °C during normal operation. The center plate, accessible at the sides and end of the Cleanstream H3000, may reach 250 °C during normal operation.



**CAUTION**

The red CAUTION equilateral triangle symbol appears throughout the manual. Please follow the important instructions accompanying this symbol to avoid significant damage to the chiller.



**WARNING**

The red WARNING equilateral triangle symbol appears throughout the manual accompanying certain maintenance and repair activities. Please follow the important instructions accompanying this symbol to avoid situations that could cause injury to the operator or other personnel.



**DANGER**

The red DANGER equilateral triangle symbol appears throughout the manual accompanying certain maintenance and repair activities. Please follow the important instructions accompanying this symbol to avoid injury to the operator. Only trained personnel should undertake any activity marked by the red DANGER triangle.

### CAUTION!

- The process side of the Cleanstream H3000 unit may reach temperatures of 150 °C during heating. Insulate prior to operation.
- Never remove the bolts clamping the Cleanstream unit together as irreparable damage may occur.
- Never operate the heat exchanger process fluid over 90°C.
- Never operate the Switchback Power Supply/Temperature Controller (associated with this Cleanstream H3000) over 24 amps or 144 volts.
- Never ship the Cleanstream unit with water inside the liquid cold plate as freezing temperatures may be encountered which would damage the unit.



## PRODUCT MANUAL

# **CLEANSTREAM H3000**

## HIGH PURITY/CORROSIVE FLUID HEATER

### 1.0 INTRODUCTION

---

The Cleanstream H3000 Heater directly heats high purity or corrosive fluids in an in-line system. All process fluid wetted parts are fabricated from PFA Teflon.

A complete system consists of the Cleanstream H3000 and a Switchback 6600CE Power Supply or Switchback 6600 Power Supply/Temperature Controller (see separate manual), which when interfaced to a PID temperature controller, can control process fluid temperatures to within  $\pm 0.1$  °C.


## 2.0 SPECIFICATIONS

Operating Range (Set Point):	40°C to 90°C
Ambient Temperature Range:	10°C to 40°C non-condensing
Stability / Repeatability:	±0.2°C with constant load
Heating Capacity (typical <sup>1</sup> ):	3000 Watts
Process Fluid:	Ideal for H <sub>2</sub> SO <sub>4</sub> / H <sub>2</sub> O, SC1, SC2 electroplating baths or other PFA Teflon compatible fluid
Process Fluid Fittings:	(see options)
Process Fluid Flow Rate:	4-10 gpm (15-38 lpm) with parallel flow (4:1 fittings) 2-4 gpm (8-15 lpm) contact SSCS 0.5-2 gpm (2-8 lpm) with series flow (Low flow Option)
Maximum Pressure:	Process: 90 psig @ 40°C, 55 psig @90°C
Wetted Materials:	Process: HDPFA Teflon
Dimensions (L x W x H):	17.5" x 11.25" x 4.65" (44.4 cm x 28.6 cm x 11.8 cm) with insulation 16" x 9.75" x 3.15" (40.6 cm x 24.8 cm x 8.0 cm) without insulation
Weight:	40 lbs (18 kg)
Power Requirements:	Switchback 6600 set to 0-144 VDC, 0-24 Amps
Standards	Semi S2-0200, F47 compliant, CE

Note 1: Heating capacity may vary with configuration

<b>Teflon Manifold Options:</b>	
-0	No manifold
-1	4x1 Fitting, 1" Weld Stub PN 32-11315-1 (set of 2)
-2	4x1 Fitting, ¾" Flaretek PN 32-11315-2 (set of 2)
-3	4x1 Fitting, 1" Flaretek PN 32-11315-3 (set of 2)
-8	Low Flow Option w/U-tubes PN 30-22840-1 (x3) and PN 30-22841-1 (x3)
<b>Insulation Options:</b>	
-IH	Silicone Insulation for Cleanstream 3000

**Figure 1 Cleanstream H3000 Pressure Drop vs Flow Rate  
(water @ 20 deg C)**

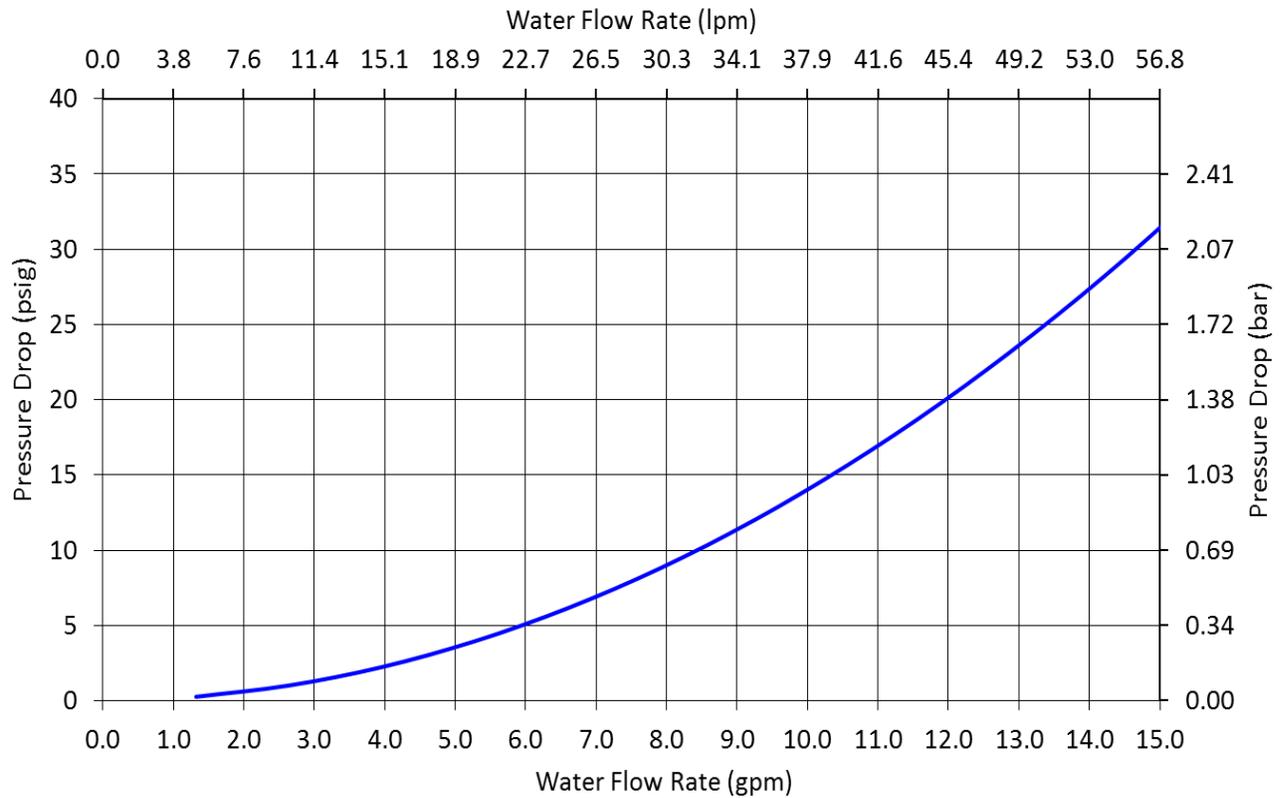

### 3.0 INSTALLATION



**WARNING**  
SSCS recommends choosing the insulation option to protect the user from potentially hot surfaces


Proper installation requires:

- 1) Mounting the Cleanstream either vertically (electrical connections at the top) or with its large flat surface horizontal per section 3.3.
- 2) Properly connecting the thermostat interlocks to the Switchback power supply per section 3.1 and figure 4.
- 3) SSCS recommends purchasing the insulation option to protect operators from hot surfaces.
- 4) SSCS also recommends the user place a leak detector under the Cleanstream process and house fluid connections to shut down the circulating fluids in the event of a leak.
- 5) Reviewing all process chemical hazards (flammability and toxicity) and insuring in the event of a leak, toxic fumes cannot come in contact with operators and, when flammable chemicals are used, no surfaces exceed the chemical's flash point and exhaust flow prevents vapor concentrations from reaching their lower explosive limits.

### 3.1 Electrical Connections

All electrical connections to the Cleanstream H3000 come through a Hummel connector PN 7.621.000.000. A single 5m (16ft) cable is provided to connect the Cleanstream to a Switchback 6600 CE power supply or Switchback 6600 CE power supply/temperature controller. The mating connector on this cable is a Hummel right-angle receptacle PN 7.576.500.000. This cable is described in Figure 2 and Table 1.

Figure 2

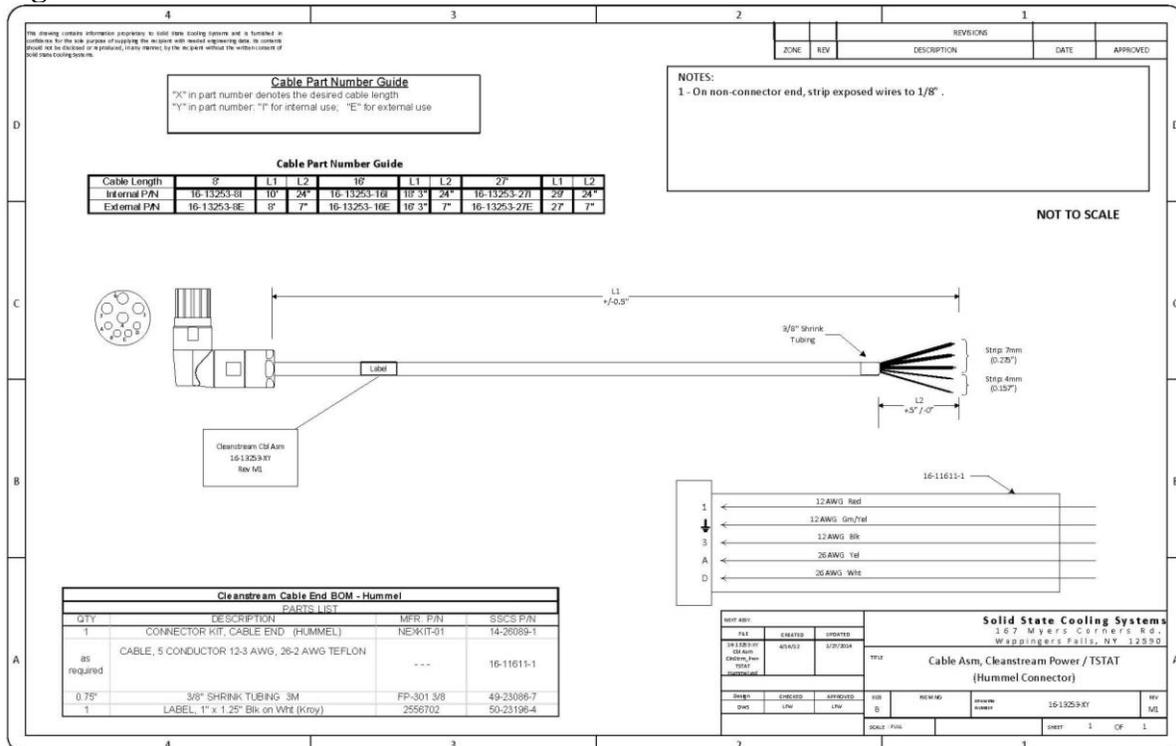



### WARNING

Failure to connect the Cleanstream thermostat wires to the Switchback Local On/Off signal will cause the Cleanstream surfaces to become excessively hot when process fluid flow is lost. This will create a burn hazard and lead to premature failure of the Cleanstream

**Table 1**

Pin#	Wire Color	Wire Size	Description
1	RED	12 AWG	DC(+) to TEC's or Heaters
3	BLK	12 AWG	DC(-) to TEC's or Heaters
↓	GRN/YEL	12 AWG	Earth Ground
A	YEL	26 AWG	Over Temperature Thermostat
D	WHT	26 AWG	Over Temperature Thermostat

**The Switchback Power Supply/Temperature controller maximum current dip switch is preset to 24A and the maximum voltage dip switch is preset to 144 VDC.**

Thermostats: The green and white 12 AWG wires connect to two thermostats for shutting down the thermoelectric system in the event of a temperature excursion on the process fluid plate. The two thermostats are wired in series and trip as follows: 177 °C normally closed, reset at 157 °C, one on each process plate.

**Important:** When using the Cleanstream unit in conjunction with the Switchback 6600 CE power supply, wire the thermostats in series with the LOCAL ON/OFF signal (even if running in remote mode).

See Figure 4 for the typical electrical hook-up from these thermostats to a Switchback 6600 power supply or power supply/temperature controller.

**Important:** Older Cleanstream systems may have different style electrical connectors for Switchback hookup (16 pin or 4 pin Fisher connectors). Please contact Solid State Cooling Systems for information on these older style connectors.

### 3.2 - Plumbing Connections

Process fluid connections are eight 3/8" x 0.030" PFA tubes, four inlet and four outlet. Two 4 x 1 PFA/PTFE reducer fittings (3/8" x 3/4" or 3/8" x 1") are also included to facilitate hook-up. (See Drawing # 19-11347-2.)

NOTE: The maximum process pressure is 2.75 bar (40 psig).

While it is the customer's responsibility to use materials compatible with the process chemistry they are using, we recommend the customer use 3/4" or 1" PFA Teflon tubing to connect to the Cleanstream 4x1 fittings. PFA Teflon is resistant to almost all chemicals and has lower diffusivity than other Teflon materials. The only exception is fluorinated heat transfer fluids such as Fluorinert, Novec, or Galden fluids which can buildup a substantial static charge when flowing through PFA Teflon.

### 3.3 - Mechanical Layout/Mounting

The Cleanstream H3000 may be mounted in any orientation for operation, though mounting the unit with the PFA Teflon tubes exiting the top will make draining the unit for servicing very difficult. The preferred orientation is horizontal or vertical with the PFA tubes exiting the side. The Cleanstream H3000 comes with eight (8) 10-32 mounting holes located on the end opposite the electrical connections. Alternatively, the Cleanstream H3000 may be placed inside an enclosure made of PVDF or other fire-retardant plastic resistant to the process chemicals or may be clamped or strapped to any frame that can support 40 lbs. (18 kg).

### 3.4 – Recommended Safety Precautions



Failure to provide leak detection or sufficient exhaust air can lead to hazardous toxic and flammable conditions in the event of a leak.

When flammable process fluids are used, failure to prevent leaks from contacting surfaces at or above the flash point of the chemical can lead to fires in the event of a leak.

The user must review the combustible and toxic properties of all process fluids and take all precautions necessary to protect operators against leak. This includes meeting all governmental regulations and industry standards.

#### 3.4.1 Leak Detection

Solid State Cooling Systems (SSCS) recommends installing liquid and, when highly toxic or flammable process chemicals are used, gas leak detectors in the enclosure where the Cleanstream is mounted. In the event of a leak, the leak detector should automatically shut down the process fluid flow and issue an alarm to the operators.

#### 3.4.2 Combustible Fluids

The user must review the combustible properties of all process fluids. The user is responsible for providing sufficient cabinet exhausting to ensure any process fluid leaks cannot cause explosive gas mixtures to occur. In addition, the enclosure housing the Cleanstream should not have any surfaces at temperatures above the flash point of the process fluid.


#### 3.4.3 Exhaust Recommendations

SSCS recommends placing the Cleanstream inside an enclosure with a chemically scrubbed exhaust with a flow rate that conforms to Semi S2 requirements and secondary containment of the process chemicals should a leak occur. The Cleanstream contains continuous pieces of PFA Teflon tubes, so internal leaks are very rare. The most likely source of leaks is improperly tightened plumbing fittings.


#### 3.4.4 Seismic Recommendations

If the Cleanstream H3000 is to be operated in a seismically active area, SSCS recommends mechanically clamping the it to a rigid structure with metal bars or fastening it to a rigid structure via the eight (8) 10-32 mounting screws. Using the top left view of 19-11347-2 (next page), the Cleanstream H3000's center of mass is located 6.75" from the right edge (opposite the electrical connector), at the midpoint of the 9.73" dimension, and halfway down into the 3.15" thickness.

Figure 3 Mechanical Layout

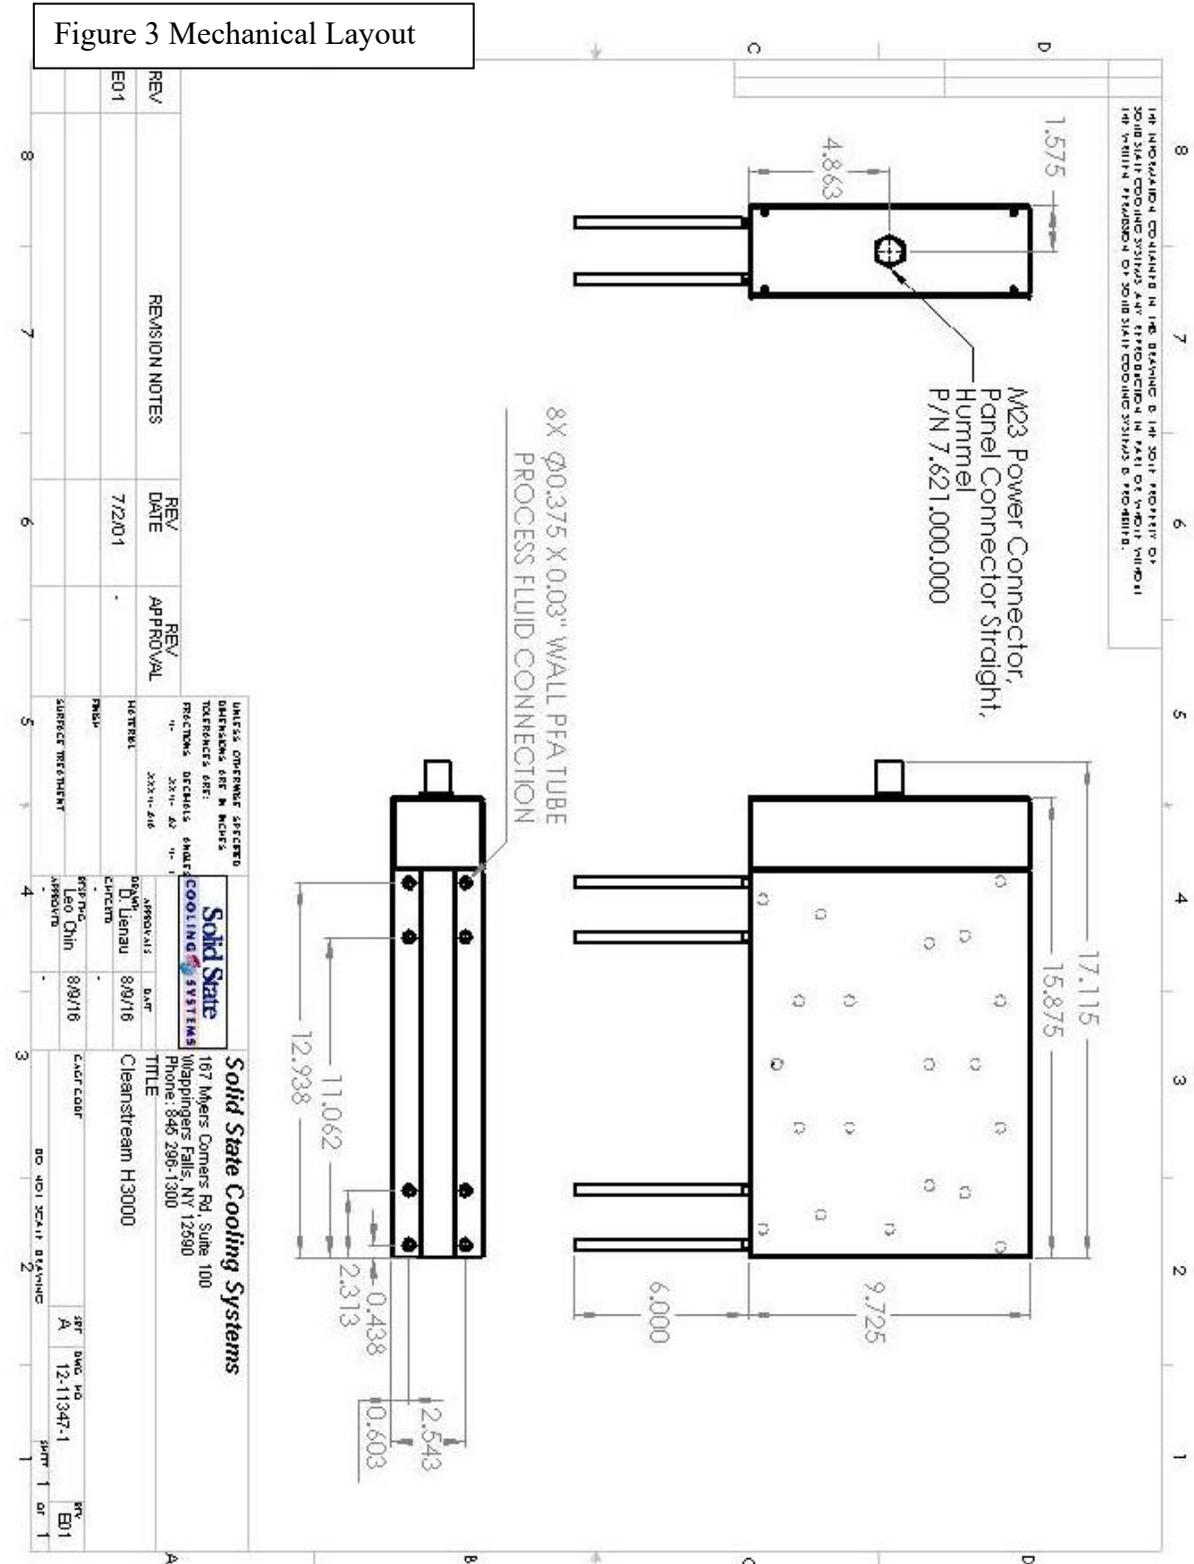

**Figure 4 Electrical Hook-up**

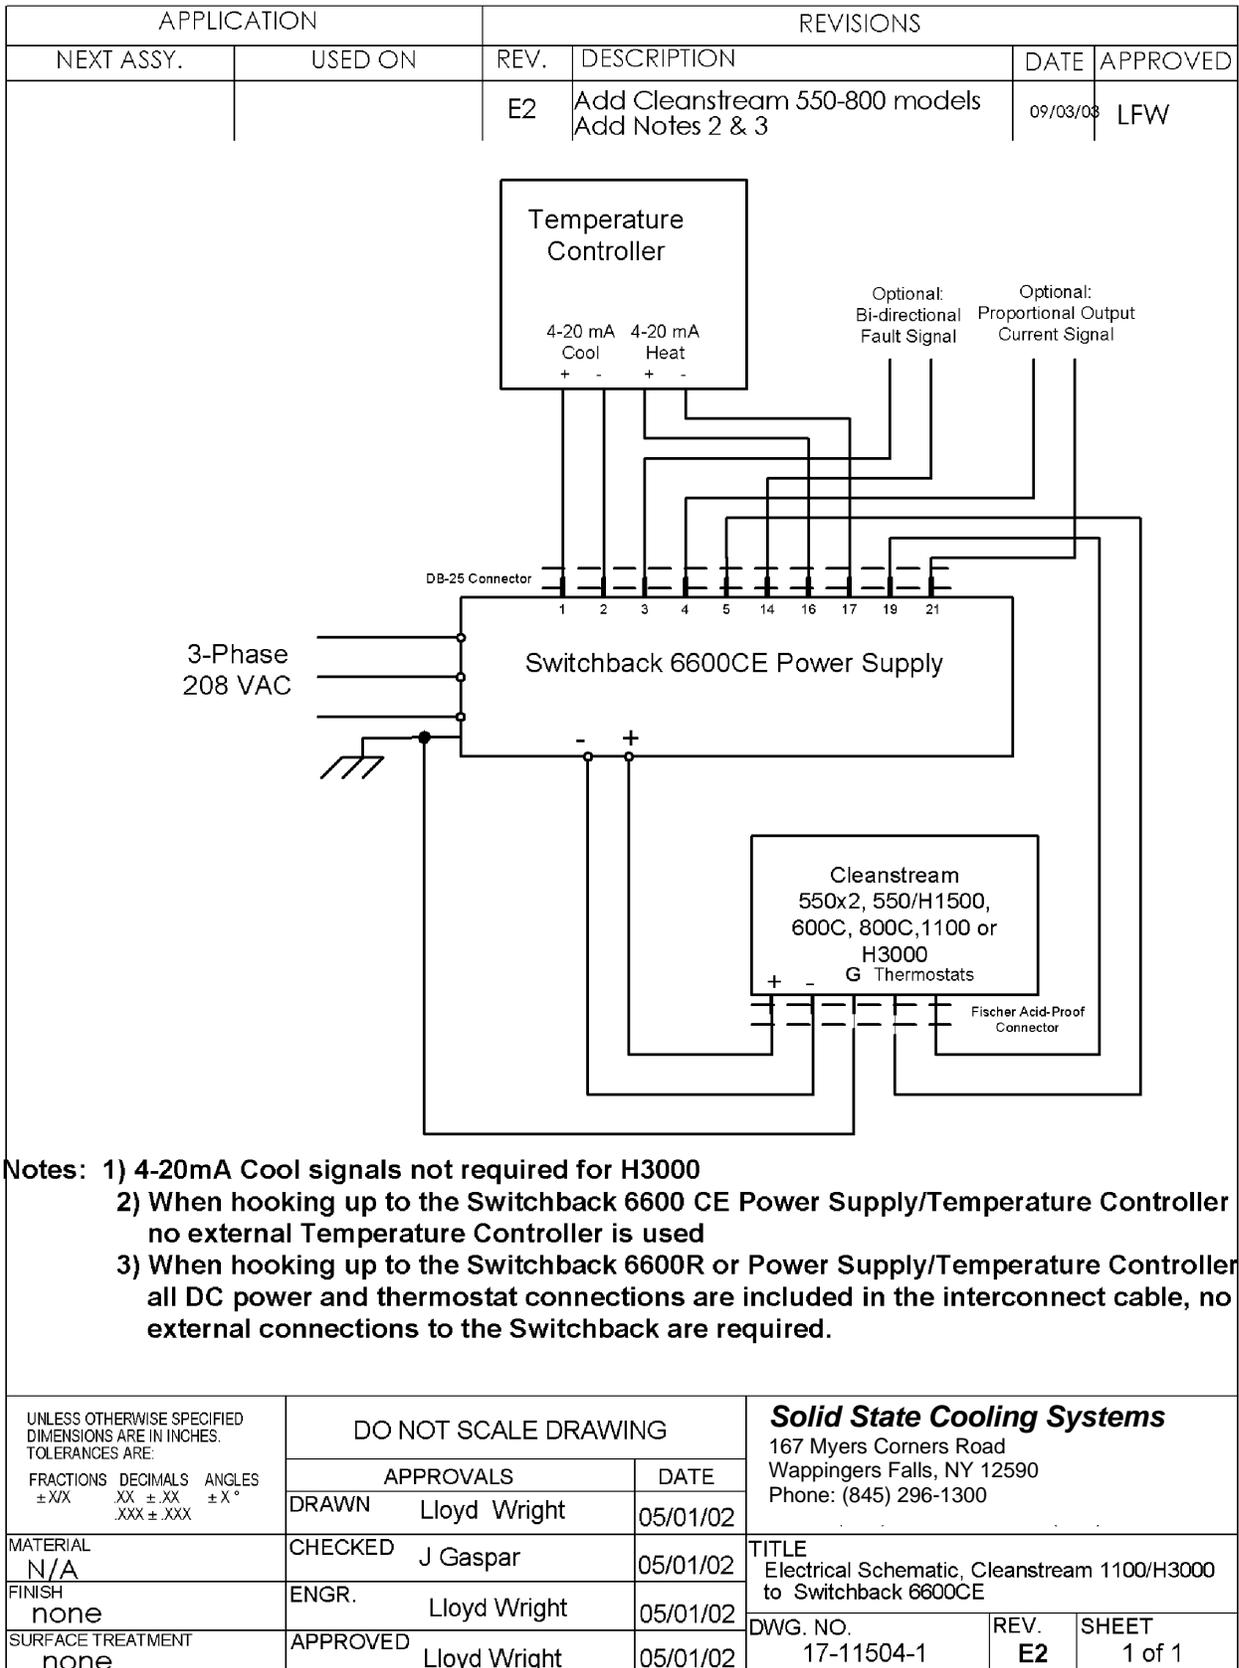

## 4.0 START-UP/OPERATION

---

Install and start the Cleanstream H3000 by following the steps below:



**DANGER**

Perform leak checking with water, not process chemicals.

- 1) Connect the 4:1 PFA reducer fittings to the two sets of PFA process fluid tubes.
- 2) Leak check the PFA fittings.
- 3) Connect the power/thermostat cable 16-13253-XY to the Switchback 6600 power supply or power supply/temperature controller as shown in Figure 4.
- 4) Plug female electrical connector (Hummel right-angle receptacle PN 7.576.500.000) into the male connector on the Cleanstream; this connected is keyed and will only plug in if correctly aligned. Rotate the latching collar while applying light pressure on the plug until the collar latches in place.
- 5) Turn on the process fluid flow.
- 6) Turn on power supply circuit breaker.
- 7) Begin operation. See Switchback 6600 Power Supply manual for details.

**Important: Observe the following warning symbols on the Cleanstream H3000:**



Burn Hazard -- Hot Surface. Top and bottom surface temperatures of the Cleanstream H3000 may reach 150 °C during normal operation. The center plate, accessible at the sides and end of the Cleanstream H3000, may reach 250 °C during normal operation.

Do Not Touch. Severe burns may occur due to hot surfaces. See above.

## 5.0 MAINTENANCE



**DANGER**

Read the SDS's for all process chemicals and take all recommended precautions prior to decontaminating a Cleanstream H3000.

The Cleanstream H3000 does not require any routine maintenance. Before removing the Cleanstream from a system that contains corrosive or toxic chemicals, disconnect power via the lockout/tagout procedure below, then use the following decontamination procedure:

- 1) Flush all tool plumbing lines with DI water until all toxic or corrosive chemicals have been removed.
- 2) Disconnect the Cleanstream 4x1 fittings from the tool.
- 3) Connect the Cleanstream 4x1 Fittings to DI water. Flush the Cleanstream for 30 minutes at a flow rate of at least 2 gpm (8 lpm).
- 4) Using a clean-room wipe soaked in DI water, wipe all exterior surfaces of the Cleanstream to remove any chemical residue.
- 5) Dry the exterior surfaces with clean-room wipes. Isopropyl alcohol may be used to speed the drying process.

## 6.0 LOCKOUT/TAG-OUT



**DANGER**

While the electrical connectors on the Switchback power supply are touch safe, hazardous voltages are present.

### Lock Out

Lock out the DC power to the Cleanstream via the following procedure:

- 1) Disconnect AC power from the Switchback 6600 by turning off the customer supplied electrical disconnect.
- 2) Unlatch the DC power plug from the Cleanstream.
- 3) Place a safety padlock through the main AC power connector to the Switchback 6600 so AC power cannot be plugged into the Switchback with the padlock in place.

### Tag Out

When locking out the main AC power receptacle, place a lockout tag through the main AC power connector latch to identify contact person/phone number. Never attach a lockout tag without first locking out the connector latch with a padlock.

## 7.0 TECHNICAL SUPPORT

---

Delighting our customers is our highest priority. Please contact us immediately for technical assistance whenever you have questions or concerns. We can be reached in New York State by telephone at (845) 296-1300, by fax at (845) 296-1303 or via e-mail at: [info1@sscooling.com](mailto:info1@sscooling.com).

## WARRANTY POLICY

---

Solid State Cooling Systems offers a full parts and labor warranty on its products. The length of a warranty is product-specific, depending on the type and planned usage of the product, but will be specified in the quotation upon which a purchase order is made. Prototypes are not warranted, but will be repaired/adjusted after original shipment until they meet the agreed-upon specifications. Malfunctioning products should be returned to Solid State Cooling Systems by the method described below. Solid State Cooling Systems will provide a Failure Analysis Report to the customer and will determine if the problem is covered under the warranty.

### Warranty Coverage:

Products with defects in components or manufacturing which are reported to Solid State Cooling Systems before the end of the warranty period will be repaired or replaced at no cost (see below for reporting requirements). The warranty period begins on the date the product was initially shipped from Solid State Cooling System's factory.

### Excluded from Warranty:

Excluded from warranty is any damage caused to the product occurring during, but not limited to, such events as shipment, installation, storage, or usage occurring during a situation specifically cautioned against or noted in the product manual.

Specific situations which invalidate the warranty include (but are not limited to):

- Removing the serial number label.
- Any disassembly (partial or complete) of a heat exchanger, which includes removing the tape on the sides, loosening or removing the bolts, or separating the heat sinks.
- Subjecting a heat exchanger to temperatures below the freezing point of the heat transfer fluid contained inside the unit.
- Subjecting a heat exchanger to unfiltered water.
- Subjecting any product to temperature, voltage, current, or pressure (internal or external) greater than that specified in the product manual.
- Employing pulse-width-modulated control at less than 1000 Hz.
- Any actions prohibited in the "Caution" section of the product manual.

### Returned Goods Procedure and Reporting Requirements

Before a failed product is returned to the factory, a Returned Materials Authorization (RMA) number must be obtained from Customer Service at (845) 296-1300. The date the RMA is requested will be the reporting date noted and relevant to the warranty. Products, which have received an RMA, must be received at Solid State Cooling System's factory within 30 days or the reporting date will be moved ahead 30 days and a new 30-day waiting period will begin.